

AT1322, AT1322/1 Whole Body Counters

*¹³¹I and ¹³³I radionuclides
measurement in human
thyroid gland*



AT1322 and AT1322/1 scintillation Whole Body Counters (WBC) are fixed instruments for measurement of ¹³¹I and ¹³³I radionuclides content in human thyroid gland.

Operating principle

WBC operating principle is based on detection of gamma-radiation from ¹³¹I and ¹³³I isotopes present in human thyroid gland by spectrometric detecting unit, and processing of instrument spectra on PC by dedicated software tools.



Joined version of AT1322 and
AT1316/AT1316A

Applications

Measurement of incorporated ¹³¹I and ¹³³I radionuclide content in thyroid gland for individual dosimetric monitoring of internal exposure, taking into account age of target person

- Laboratory for internal exposure monitoring of nuclear power plants and other enterprises staff and citizens in the event of radionuclide ingress into human body
- Radiation diagnostic laboratories in health care facilities

Features

- High examination rate: 3 minutes per person
- Automatic LED stabilization of WBC energy scale
- Flexible software control of WBC functions, generation of database and report based on measurement results
- Compact design
- USB Counter-to-PC connection
- Can be operated independently or together with AT1316/AT1316A, as well as part of mobile spectrometric laboratory



ATOMTEX[®]

INSTRUMENTS AND TECHNOLOGIES FOR NUCLEAR
MEASUREMENTS AND RADIATION MONITORING


AT1322, AT1322/1 Whole Body Counters

Specification

Detector type AT1322 AT1322/1	Scintillator, NaI(Tl) ø40x40 mm NaI(Tl) ø63x63 mm
Registered gamma radiation energy range AT1322, AT1322/1	50 keV...1.5 MeV
Minimum measured activity of ¹³¹ I and ¹³³ I in human thyroid gland for 3 min. measurement interval	
¹³¹ I (AT1322)	200 Bq
¹³¹ I (AT1322/1)	80 Bq
¹³³ I (AT1322)	240 Bq
¹³³ I (AT1322/1)	100 Bq
Radionuclides activity measurement range in human thyroid gland	
¹³¹ I (AT1322)	85...10 ⁵ Bq
¹³¹ I (AT1322/1)	30...10 ⁵ Bq
¹³³ I (AT1322)	110...10 ⁵ Bq
¹³³ I (AT1322/1)	40...10 ⁵ Bq
Number of ADC channels	512
Integral nonlinearity	±1% max.
Typical resolution at 662 keV (¹³⁷Cs)	7.5%
Measurement instability during continuous service	±3% max.
Operation mode setup time	10 min
Continuous run time	24 h
Express-monitoring productivity	15 person/h
Working temperature range	+10°C...+35°C
Relative humidity with air temperature ≤30°C without condensation	≤75%
Power supply	110-230 VAC, 50-60 Hz
Power consumption	≤200 VA
Weight	70 kg

Design and specifications are subject to change without notice

Measurement result display

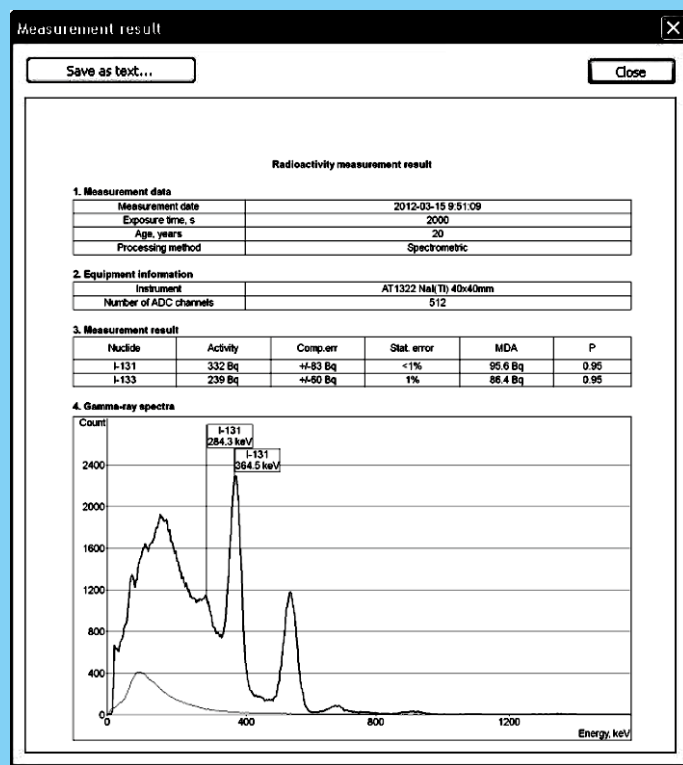

AT1322 and AT1322/1 Whole Body Counters meet Safety standard requirements:

IEC 61010-1:2001

EMC requirements:

EN 55011:2009

IEC 61000-4-2:2008

IEC 61000-4-4:2006

IEC 61000-4-5:2005

IEC 61000-4-11:2004




ATOMTEX®

<http://www.atomtex.com>

5, Gikalo st., 220005 Minsk,
Republic of Belarus

Tel./fax: +375 17 2928142

E-mail: info@atomtex.com



ENr
Corporate Member
of European
Nuclear
Society